



# Amino and PEG-amino graphene oxide grids enrich and protect samples for high-resolution single particle cryo-electron microscopy

Feng Wang<sup>a,1</sup>, Zanlin Yu<sup>a,1</sup>, Miguel Betegon<sup>a</sup>, Melody G. Campbell<sup>a</sup>, Tural Aksel<sup>b</sup>, Jianhua Zhao<sup>a</sup>, Sam Li<sup>a</sup>, Shawn M. Douglas<sup>b</sup>, Yifan Cheng<sup>a</sup>, David A. Agard<sup>a,\*</sup>

<sup>a</sup> Department of Biochemistry & Biophysics and the Howard Hughes Medical Institute, University of California, San Francisco, San Francisco, CA 94143, United States

<sup>b</sup> Department of Cellular and Molecular Pharmacology, University of California, San Francisco, San Francisco, CA 94158, United States

## ARTICLE INFO

### Keywords:

Cryo-EM  
Graphene oxide  
Sample preparation  
Amino functionalization  
Air-water interface

## ABSTRACT

Cryo-EM samples prepared using traditional methods often suffer from too few particles, poor particle distribution, strongly biased orientation, or damage from the air-water interface. Here we report that functionalization of graphene oxide (GO) coated grids with amino groups concentrates samples on the grid with improved distribution and orientation. By introducing a PEG spacer, particles are kept away from both the GO surface and the air-water interface, protecting them from potential denaturation.

## 1. Introduction

Single particle cryo-electron microscopy (cryo-EM) has become a major method for determining protein structures at a near-atomic or atomic resolution (Cheng, 2015; Nogales, 2016). Despite rapid advances in image collection and processing, sample preparation has remained largely unchanged, and can be rate limiting. In the standard cryo-EM specimen preparation process, the protein sample is applied onto a holey cryo-EM grid and the grid is plunged into liquid ethane after blotting to obtain a thin layer of vitrified amorphous ice, in principle, preserving the biological sample in a hydrated state (Mcdowall et al., 1983; Taylor and Glaeser, 1974). In practice, however, there are many issues preventing a sample from being in an ideal state for data collection. First, some particles strongly prefer to stick to the carbon film instead of being visible within the holes (Snijder et al., 2017). Second, some proteins cannot be concentrated to a sufficient level for cryo-EM sampling. Third, proteins or complexes may adopt “preferred orientations”, dissociate or denature as a result of interactions with the air-water interface (D’Imprima et al., 2019; Tan et al., 2017). This is now understood to be a much more pervasive problem than originally thought (Noble et al., 2017). Numerous approaches have been aimed at combatting these problems, including PEGylation on gold coated holey carbon grids (Meyerson et al., 2014), addition of detergents (Chen et al., 2019), use of grids deposited with a thin continuous carbon film (Nguyen et al., 2015) or surface modified graphene as substrate (D’Imprima et al., 2019; Naydenova et al., 2019), collecting

data at defined tilts (Tan et al., 2017) and so on. However, no single strategy has yet to be widely adopted due to technical challenges, cost of materials, requirements for highly specialized equipment to make single crystal graphene films, or the deterioration of signal-to-noise and resolution experienced with thin carbon films.

To circumvent these problems, we first developed a simple and convenient approach to efficiently deposit graphene oxide (GO) films on EM-grids (Palovcak et al., 2018), and have since explored various strategies for chemical functionalization. Here we discuss the broad utility of amino-functionalized GO grids (Fig. 1A). The resulting grids provided a robust and broadly useful strategy for non-selectively enriching proteins on the grid. We tested four different samples and found that 1) proteins were significantly enriched, much like on negative stained carbon grids, 2) particles were nicely distributed over grid holes 3) particle orientations were altered, without being overly biased. Using the 20S proteasome, we conducted cryo-electron tomography experiments and confirmed that particles stay close to the surface of amino-GO grids, rather than being located at the air-water interface. Moreover, addition of a polyethylene glycol (PEG) spacer between the amino group and the GO surface (amino-PEG-GO grid; Fig. 1B), kept particles away from both the GO surface and the air-water interface, which may further reduce orientation bias and help preserve sample integrity.

## 2. Materials and methods

Synthesis of GO and deposition of GO onto Quantifoil EM grids were

\* Corresponding author.

E-mail address: [agard@msg.ucsf.edu](mailto:agard@msg.ucsf.edu) (D.A. Agard).

<sup>1</sup> Feng Wang and Zanlin Yu contributed equally.

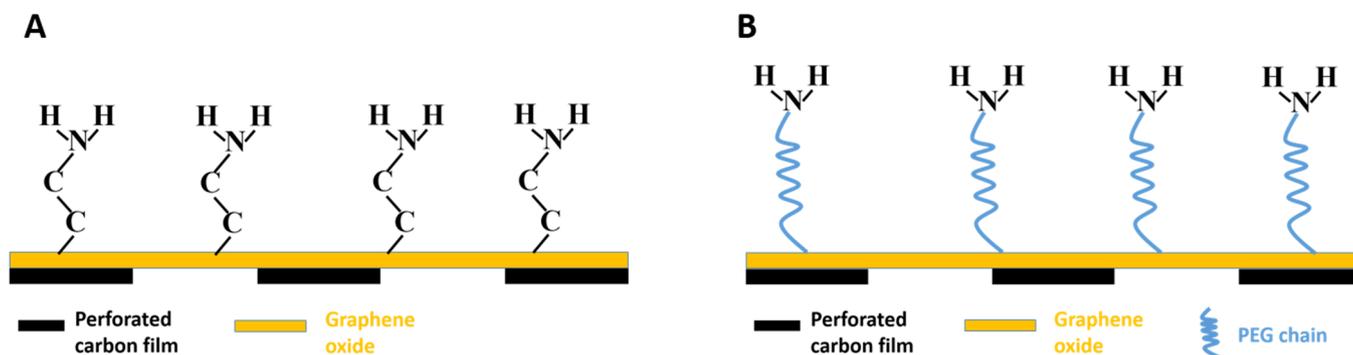


Fig. 1. Schematic illustration of (A) amino-GO grid and (B) amino-PEG-GO grid assembly.

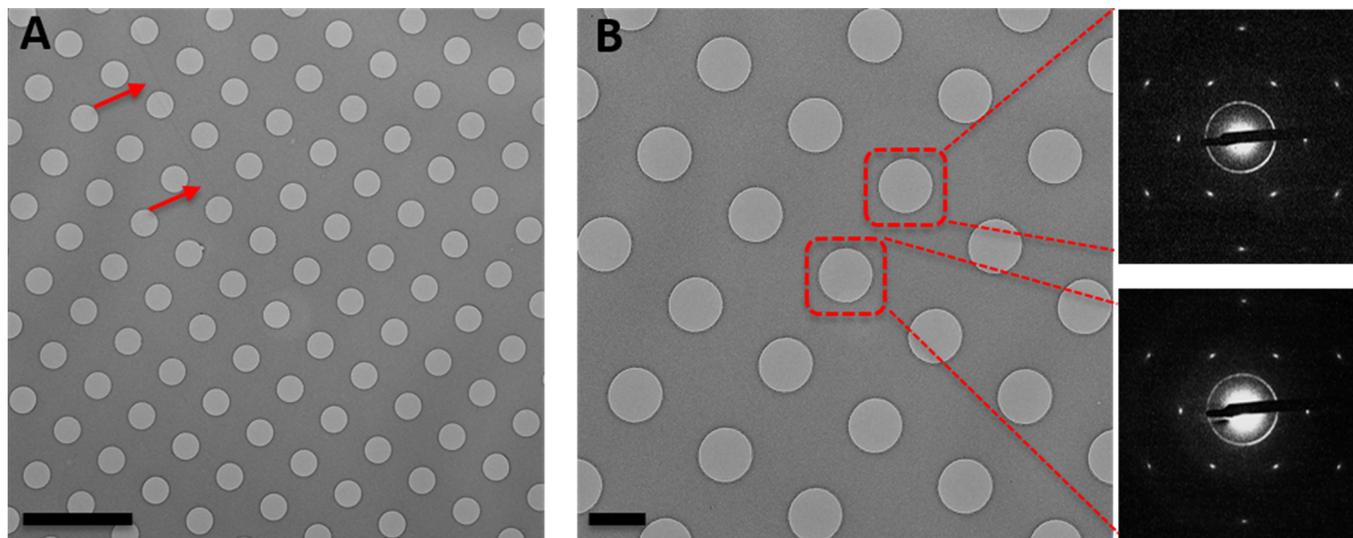


Fig. 2. Transmission electron microscope (TEM) images of an EM grid covered by GO. (A) TEM image at 2500x displaying full coverage of GO over the square. The existence of GO is confirmed by wrinkles as indicated by the red arrows. Scale bar: 5  $\mu\text{m}$ . (B) TEM image at 5000x showing GO coating of single layer. Scale bar: 1  $\mu\text{m}$ . Selected area electron diffraction (SAED) images were taken from the holes marked by dashed square.


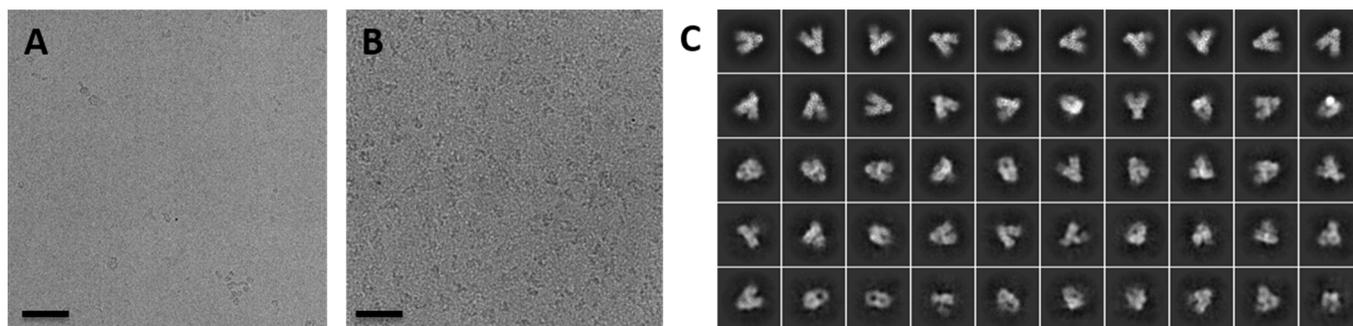


Fig. 3. Cropped cryo-EM micrographs of the complex between bacterial Hsp90 and bacterial ribosomal protein L2 on a holey carbon grid (A) and on an amino-GO grid (B). Scale bars: 50 nm. (C) Selected 2D class averages from the complex described in (B). No particles were observable on a holey carbon grid with a protein concentration of 10  $\mu\text{M}$ . By contrast, particle density was nearly ideal using an amino-GO grid with a protein concentration of 250 nM.

described in detail in our earlier work (Wang et al., 2019) and can also be found in [supplementary information](#). Surface modification of GO was designed via the nucleophilic ring opening of epoxy groups by primary amines (Luo et al., 2016). GO grids were submerged in 30  $\mu\text{l}$  of 10 mM ethylenediamine (Sigma-Aldrich E26266) solution in dimethyl sulfoxide (DMSO) and gently shaken on an Eppendorf Thermomixer for 5 h (Supplementary Fig. 1). The grids were rinsed thoroughly with deionized (DI) water three times and subsequently with ethanol two times and dried under ambient conditions. For Amino-PEG-GO grids, GO grids were submerged in 1 mM amine-PEG-amine (molecular

weight 5000 Da, Nanocs PG2-AM-5 k) solution in DMSO and gently shaken overnight. After washing with DI water three times and with ethanol two times, the amino-PEG-GO grids were air dried. Both kinds of grids should be stored dry at  $-20\text{ }^{\circ}\text{C}$  and are effective for at least months. Details of biological sample preparation and cryo-EM data collection can be found in the [supplementary information](#).

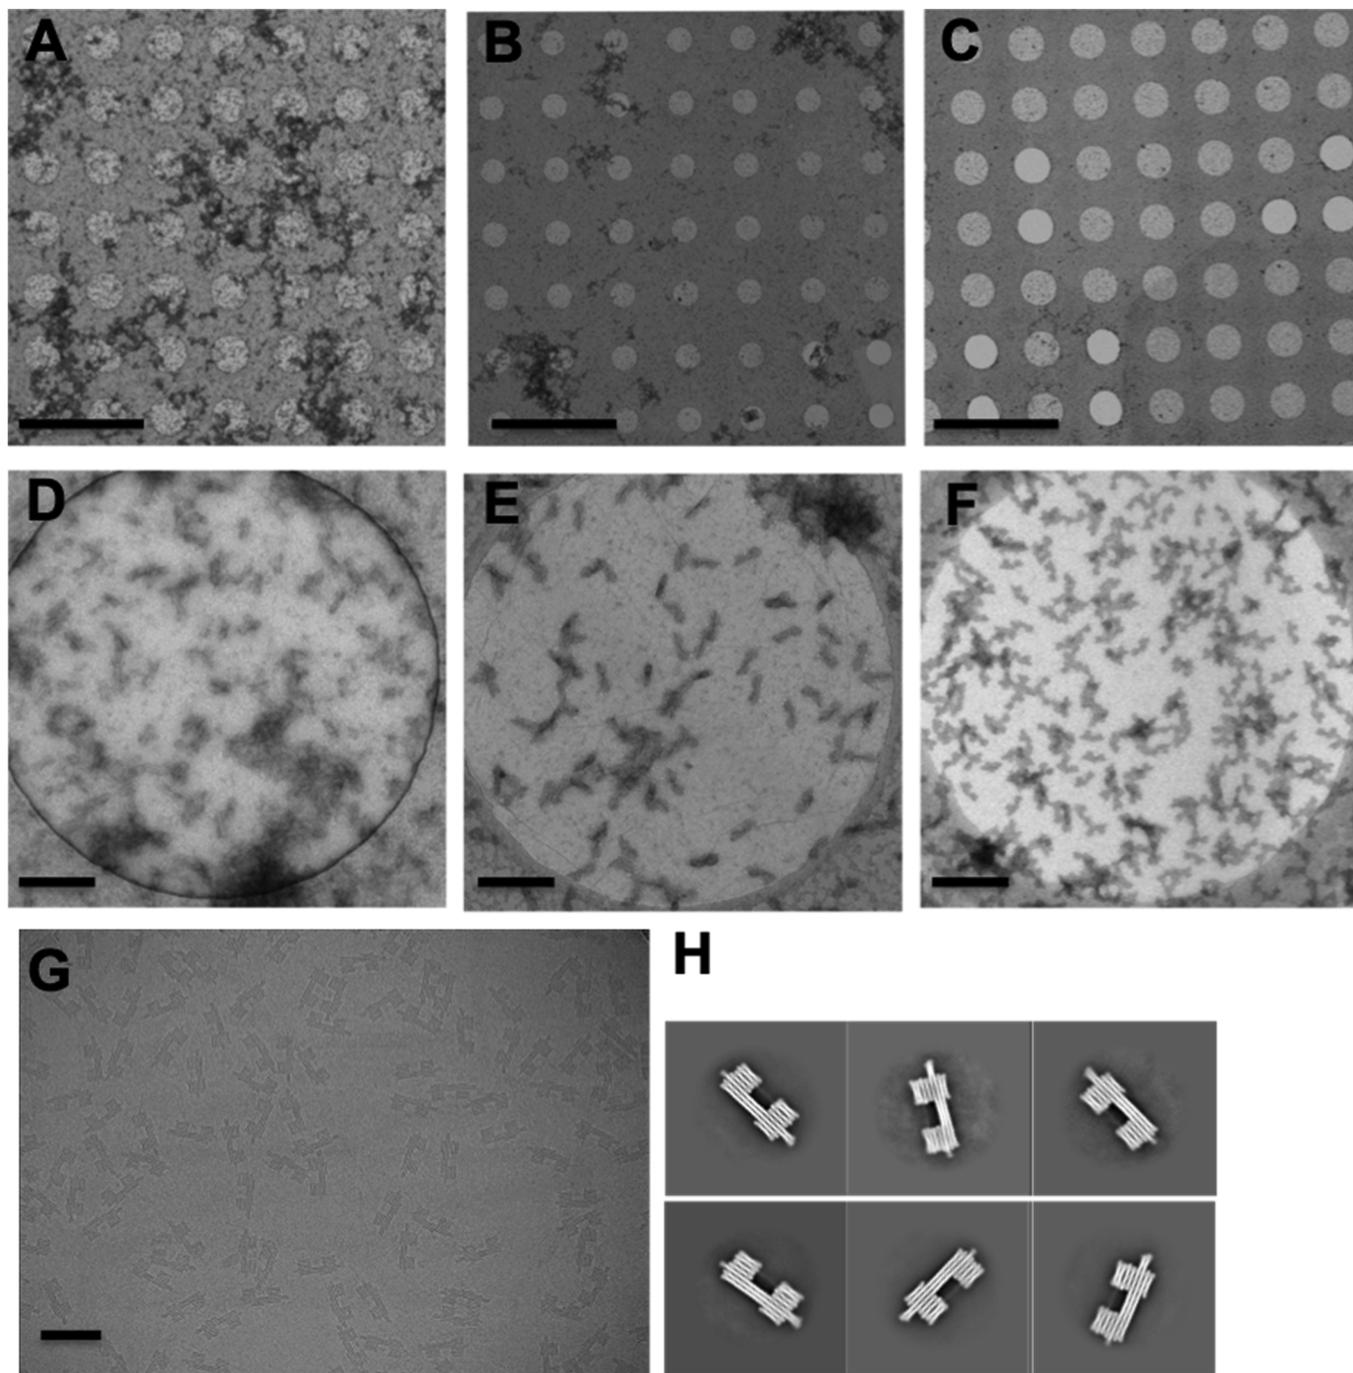

**Fig. 4.** TEM images of DNA origami structures deposited on thin amorphous carbon coated grids (A) (D), GO grids (B) (E) and amino-GO grids (C) (F) from negative stain sampling. (G) A cryo-EM micrograph showing DNA origami structures observed on an amino-GO grid. (H) Selected 2D class averages of DNA origami structures from (G). Scale bars in (A), (B) and (C): 5  $\mu\text{m}$ . Scale bars in (D), (E) and (F): 200 nm. Scale bar in (G): 100 nm. DNA origami structures aggregated severely on both thin amorphous carbon coated grids and unmodified GO coated grids, but dispersed well on amino-GO grids. For this sample, it was desired that all structures lay flat as observed with amino-GO grids (G).

### 3. Results and discussions


#### 3.1. GO coating on EM grid

As demonstrated in our previous work (Wang et al., 2019), GO deposition using the Langmuir-Blodgett method produced robust and satisfactory coating. We estimated that GO covers over 90% of the grid surface, with at least 40% being monolayer, about 40% bilayer and rest having three layers. GO regions having more than three layers are very rare. Two representative transmission electron microscope (TEM)

images of GO coated gold Quantifoil EM grid at low magnifications are shown in Fig. 2.

#### 3.2. Improvement of protein distribution over the grid holes

We used the complex between bacterial Hsp90 and its client protein, bacterial ribosomal protein L2 (~170 kDa) to illustrate the performance of the amino-GO grid in protein distribution improvement. With Quantifoil holey carbon grids, no particles were observed inside the grid holes despite using complex concentrations as high as 10  $\mu\text{M}$

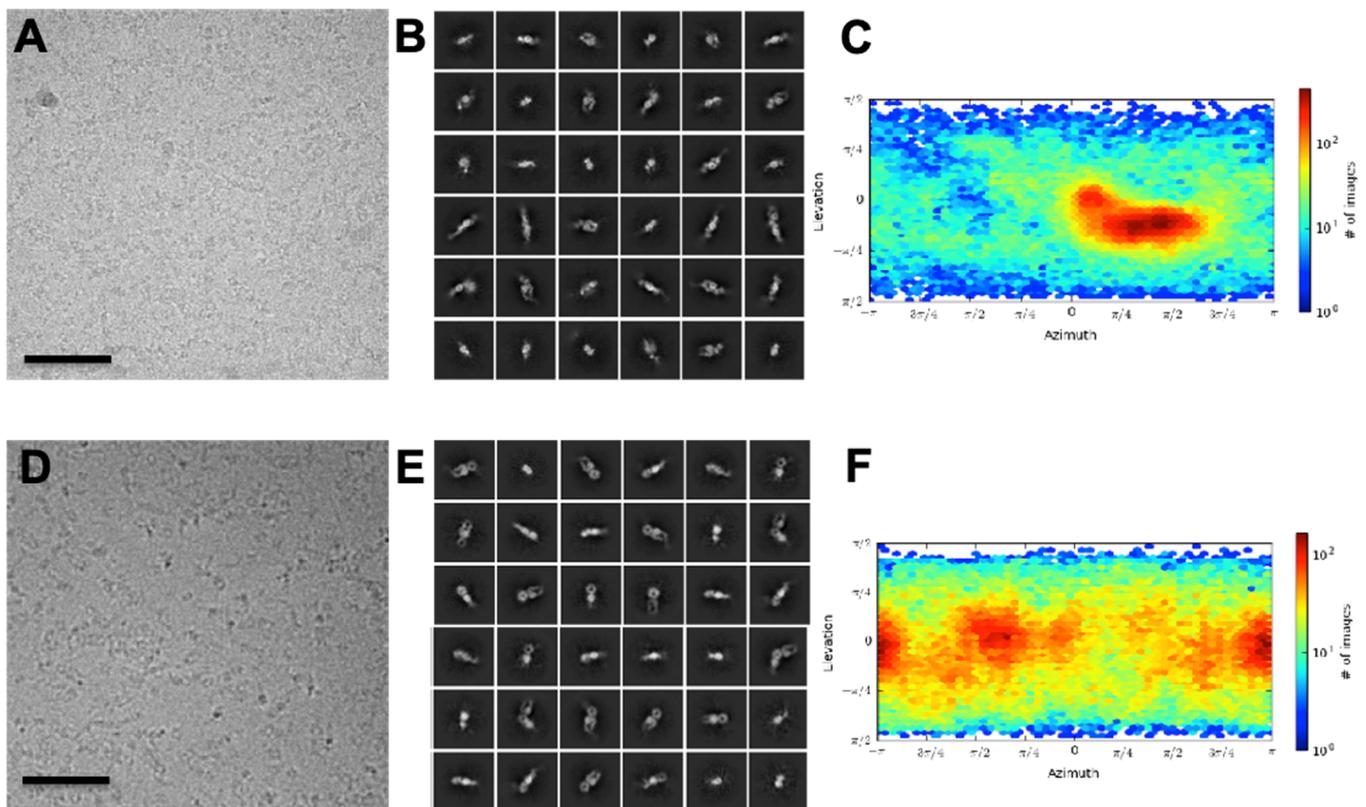

**Fig. 5.** (A) Cropped cryo-EM micrograph, (B) selected 2D class averages and (C) orientation distribution of the  $\alpha 5 \beta 8 / L$ -TGF- $\beta$  complex on traditional holey carbon grids. (D) Cryo-EM micrograph, (E) selected 2D class averages and (F) orientation distribution of the same  $\alpha 5 \beta 8 / L$ -TGF- $\beta$  complex on an amino-GO grid. Scale bars: 50 nm. Particles exhibited predominately side views on holey carbon grids. On amino-GO grids, the orientation distribution improved dramatically.

(Fig. 3A). The same sample showed ideal particle density when applied to amino-GO grids in concentrations as low as 250 nM, with excellent distribution, clearly recognizable particles and producing good 2D classes (Fig. 3B and C).

Another demonstration of improved particle distribution is evident when using a DNA origami sample. For this application, it was desired to have the DNA origami structure always land flat on its side, which requires the use of a support film on grid surface. Although a thin layer of amorphous carbon or GO film may both serve this purpose, we found that the DNA origami structures deform and make large aggregates on Quantifoil grids with thin amorphous carbon (Fig. 4A and D) or unmodified GO films (Fig. 4B and E). On the other hand, mono dispersed DNA origami structures were quite visible on amino-GO grids (Fig. 4C and F), and remained well folded even though their large area flat surfaces were in contact with the GO surface (Fig. 4G and H).

### 3.3. Change of particle orientation

We tested the integrin  $\alpha 5 \beta 8 / L$ -TGF- $\beta$  complex, which showed a set of strongly preferred orientations (predominantly side views) when frozen on traditional holey carbon grids at a concentration of 0.25 mg/ml. This resulted in 3D maps that were overestimated in resolution likely due to overfitting and highly “stretched” due to the anisotropic resolution. The complex frozen on amino-GO grids (0.075 mg/ml) gave a wider distribution of orientations, providing more top, bottom, and ‘en face’ views than the holey carbon grids, as reflected in the orientation distribution map (Fig. 5). Thus, using data from amino-GO grids was essential for obtaining a high quality map.


Another project plagued by strongly preferred orientation was TRPA1, which adopted only top views on regular holey carbon grids, preventing 3D structure determination. In order to acquire side views necessary for calculating the 3D structure, the TRPA1 sample

was prepared on amino-GO grids. As shown in Fig. 6, TRPA1 particles adhered well to the grids, but this time exhibited a predominant side view orientation. Although reconstructions can often be obtained with side view particles alone, we combined both top and side views to determine a  $\sim 3.5$  Å resolution map of TRPA1.

Considering that most particles dwell at the air-water interface with conventional holey carbon grids (Noble et al., 2017), it seems reasonable to assume the orientation change was at least in part caused by keeping particles away from air-water interface. This was confirmed by tomographic analysis. Using the 20S proteasome, on the amino-GO grid the vast majority of protein particles were pulled away from the air-water interface, likely due to a weak electrostatic interactions between the primary amines on the GO and the protein. The particles stacked continuously spanning a distance of 20 nm with the bottom layer of particles around 5 nm from the GO surface (Fig. 7A). As 20S particle are cylinder shaped, the two bands of distances likely represent perpendicular orientations with some or most particles in near contact with the amino-GO surface. In order to keep particles away from both the air-water interface and the GO surface, we introduced a PEG spacer between the capping amino groups and the GO surface. As a result, with the same amount of protein applied, few particles were found to stick to the GO surface while particle were again clustered in a band at 20–40 nm, again likely reflecting perpendicular orientations (Fig. 7B).

## 4. Conclusion

In summary, functionalizing GO grids with amino groups results in a support film for cryo-EM capable of broadly providing sample enrichment. The grid surface wettability as well as the protein distribution were greatly improved compared to bare GO grids. Moreover, the particle orientation could be changed, in part due to the ability the amino-GO grids to pull particles away from the air-water interface.

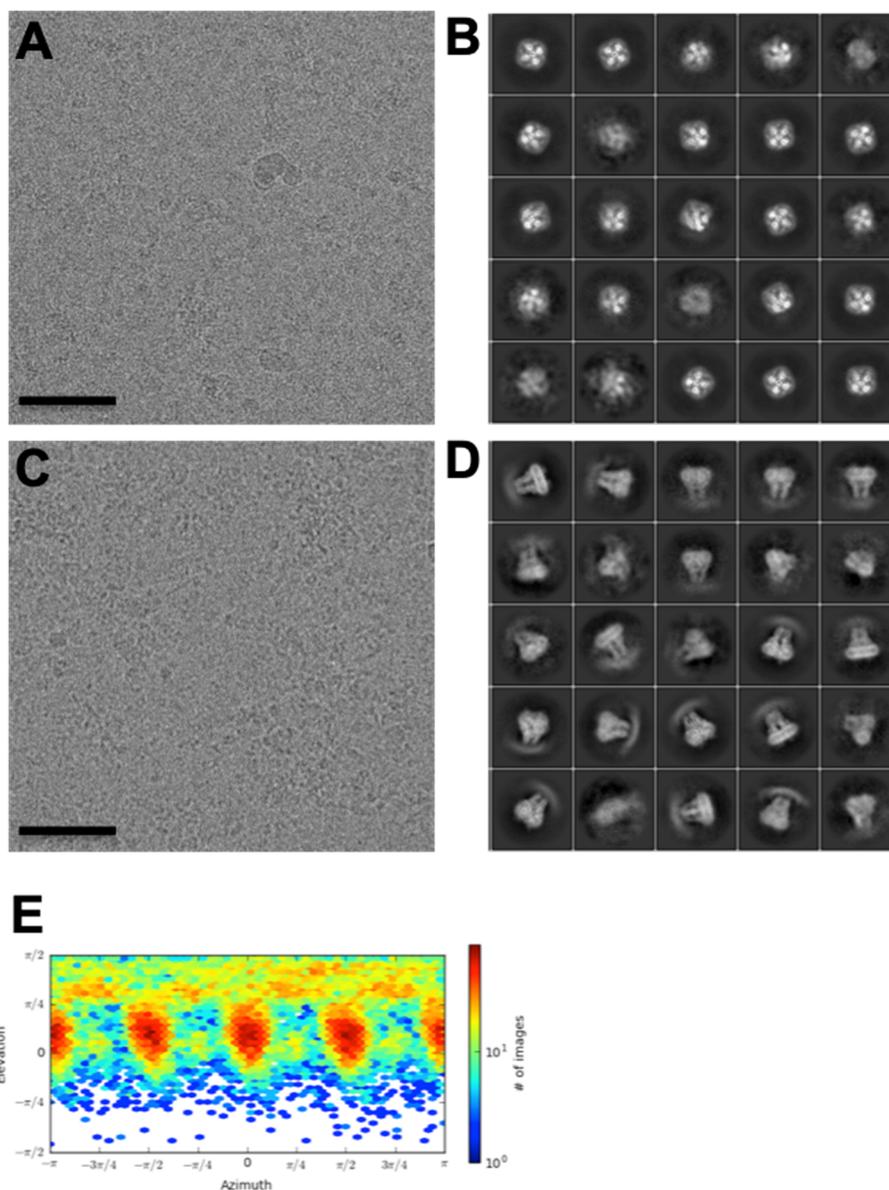

**Fig. 6.** (A) Cropped cryo-EM micrograph and (B) selected 2D class averages of TRPA1 protein on a holey carbon grid. (C) Cropped cryo-EM micrograph and (D) selected 2D class averages of TRPA1 protein on an amino-GO grid. (E) Orientation distribution map of TRPA1 protein after combining data sets from both the regular holey carbon grid and the GO-amino grid. Scale bars: 50 nm. TRPA1 adopted only top views on holey carbon grids and only side views on amino-GO grids.

Notably, addition of a PEG spacer kept particles away from both the air-water interface and the GO surface, which would further protect delicate samples from potential partial denaturation and aggregation, as well as further minimizing orientation bias due to the flexibility of the PEG chains. It is also noteworthy that while we focused on amino modifications for their general utility, GO grid surface functionalization conveniently extends to the coupling of a diverse array of moieties, i.e. carboxyl, hydroxyl, phenoxyl groups, secondary amines, DNA/RNA, hydrophilic polymers etc. to offer general affinity and adapt to a much broader range of proteins.

#### Author contribution

F.W., Z.Y. and D.A.A. designed the experiments. F.W. developed GO grids with amine functionalization. M.B. tested bacterial Hsp90 complex on amino-GO grids and collected data. T.A., Z.Y. and S.M.D. tested DNA origami on amino-GO grids and collected data. M.G.C. tested integrin  $\alpha\text{v}\beta\text{8}/\text{L-TGF-}\beta$  complex amino-GO grids and collected data. Z.Y. and S.L. conducted cryo-electron tomography. F.W. and Z.Y. wrote the

manuscript with input from all authors. Y.C. and D.A.A. supervised the project.

#### Declaration of Competing Interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

#### Acknowledgements

We wish to thank Yanxin Liu and Eugene Palovcak for helpful discussions, Michael Braunfeld, Alex Myasnikov, David Bulkley for help and running the UCSF Advanced Cryo-Electron Microscopy Facility, and Matt Harrington for HPC support. TA holds Ruth L. Kirschstein NRSA Postdoctoral Fellowship F32GM119322. SMD is supported by NIH grant R35GM125027. Funding to DAA comes from a UCSF PBBR technology development grant, and NIH grants R35GM118099, U54CA209891, U01MH115747 and U19AI135990. YC is supported by

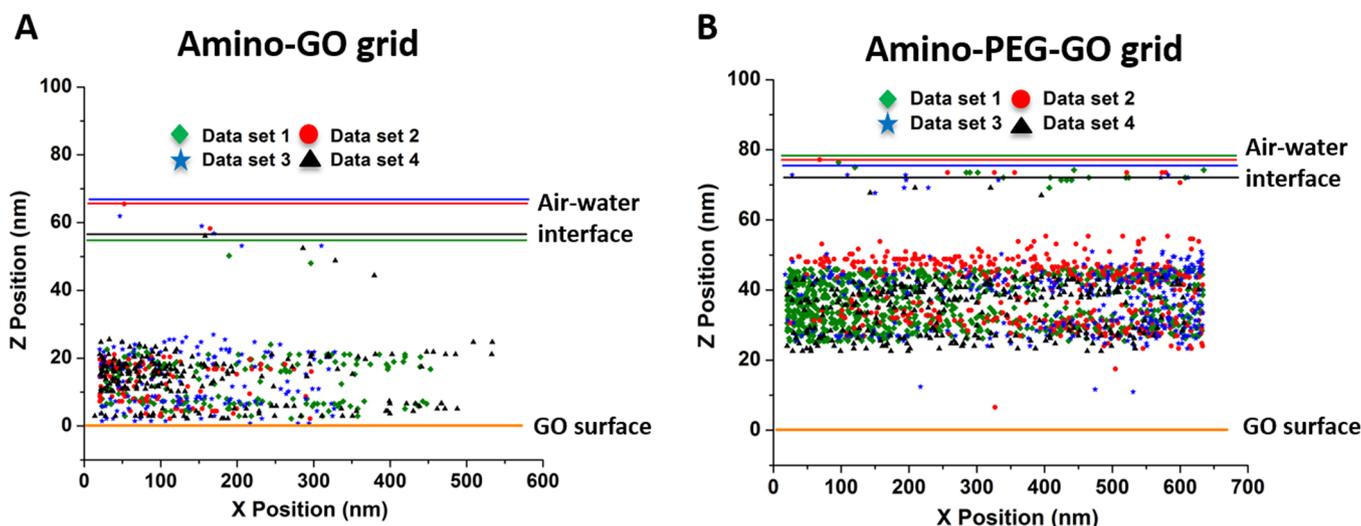


Fig. 7. Determination of particle position from within the vitreous ice layer by tomographic analysis. Localization of 20S proteasome particles on (A) amino-GO grids and (B) amino-PEG-GO grids. Particle coordinates were collected from 4 data sets and represented by markers in different colors. The GO surface is set to zero for all data sets. The location of the air-water interfaces are illustrated with lines of color corresponding to each data set.

NIH grants R01GM098672, 1R01HL134183, 1S10OD021741 and 1S10OD020054. DAA was, and YC is supported by the Howard Hughes Medical Institute, and the facility has received NIH instrumentation grants S10OD020054 and S10OD021741.

#### Appendix A. Supplementary data

Supplementary data to this article can be found online at <https://doi.org/10.1016/j.jsb.2019.107437>.

#### References

- Chen, J., Noble, A.J., Kang, J.Y., Darst, S.D., 2019. Eliminating effects of particle adsorption to the air/water interface in single-particle cryo-electron microscopy: Bacterial RNA polymerase and CHAPSO. *J. Struct. Biol.* X 1, 100005.
- Cheng, Y.F., 2015. Single-particle cryo-EM at crystallographic resolution. *Cell* 161, 450–457.
- D'Imprima, E., Floris, D., Joppe, M., Sanchez, R., Grininger, M., Kuhlbrandt, W., 2019. Protein denaturation at the air-water interface and how to prevent it. *Elife* 8.
- Luo, D., Wang, F., Zhu, J.Y., Cao, F., Liu, Y., Li, X.G., Willson, R.C., Yang, Z.Z., Chu, C.W., Ren, Z.F., 2016. Nanofluid of graphene-based amphiphilic Janus nanosheets for tertiary or enhanced oil recovery: high performance at low concentration. *Proc. Natl. Acad. Sci. U.S.A.* 113, 7711–7716.
- Mcdowall, A.W., Chang, J.J., Freeman, R., Lepault, J., Walter, C.A., Dubochet, J., 1983. Electron-microscopy of frozen hydrated sections of vitreous ice and vitrified biological samples. *J. Microsc-Oxford* 131, 1–9.
- Meyerson, J.R., Rao, P., Kumar, J., Chittori, S., Banerjee, S., Pierson, J., Mayer, M.L., Subramaniam, S., 2014. Self-assembled monolayers improve protein distribution on holey carbon cryo-EM supports. *Sci. Rep.* 4, 7084.
- Naydenova, K., Peet, M.J., Russo, C.J., 2019. Multifunctional graphene supports for electron cryomicroscopy. *Proc. Natl. Acad. Sci. U.S.A.* 116, 11718–11724.
- Nguyen, T.H.D., Galej, W.P., Bai, X.C., Savva, C.G., Newman, A.J., Scheres, S.H.W., Nagai, K., 2015. The architecture of the spliceosomal U4/U6.U5 tri-snRNP. *Nature* 523, 47–52.
- Noble, A.J., Dandey, V.P., Wei, H., Braschi, J., Chase, J., Acharya, P., Tan, Y.Z., Zhang, Z.N., Kim, L.Y., Scapin, G., Rapp, M., Eng, E.T., Rice, W.J., Cheng, A.C., Negro, C.J., Shapiro, L., Kwong, P.D., Jeruzalmi, D., des Georges, A., Potter, C.S., Carragher, B., 2018. Routine single particle cryoEM sample and grid characterization by tomography. *Elife* 7.
- Nogales, E., 2016. The development of cryo-EM into a mainstream structural biology technique. *Nat. Methods* 13, 24–27.
- Palovcak, E., Wang, F., Zheng, S.Q., Yu, Z., Li, S., Betegon, M., Bulkley, D., Agard, D.A., Cheng, Y., 2018. A simple and robust procedure for preparing graphene-oxide cryo-EM grids. *J. Struct. Biol.* 204, 80–84.
- Snijder, J., Borst, A.J., Dosey, A., Walls, A.C., Burrell, A., Reddy, V.S., Kollman, J.M., Veesler, D., 2017. Vitrification after multiple rounds of sample application and blotting improves particle density on cryo-electron microscopy grids. *J. Struct. Biol.* 198, 38–42.
- Tan, Y.Z., Baldwin, P.R., Davis, J.H., Williamson, J.R., Potter, C.S., Carragher, B., Lyumkis, D., 2017. Addressing preferred specimen orientation in single-particle cryo-EM through tilting. *Nat. Methods* 14, 793–796.
- Taylor, K.A., Glaeser, R.M., 1974. Electron-diffraction of frozen, hydrated protein crystals. *Science* 186, 1036–1037.
- Wang, F., Liu, Y., Yu, Z., Li, S., Cheng, Y., Agard, D.A., 2019. General and robust covalently linked graphene oxide affinity grids for high-resolution cryo-EM. *bioRxiv*. <https://doi.org/10.1101/657411>.